




Correction to: Knowledge distillation for efficient standard scanplane detection of fetal ultrasound

Jacopo Daputo¹ · Luca Zini² · Francesca Odone¹

Published online: 13 September 2023
 © International Federation for Medical and Biological Engineering 2023

Correction to: Medical & Biological Engineering & Computing
<https://doi.org/10.1007/s11517-023-02881-4>

The original version of this article unfortunately contained a mistake. The graphical abstract displayed in the published online version is incorrect. The correct image is shown below:

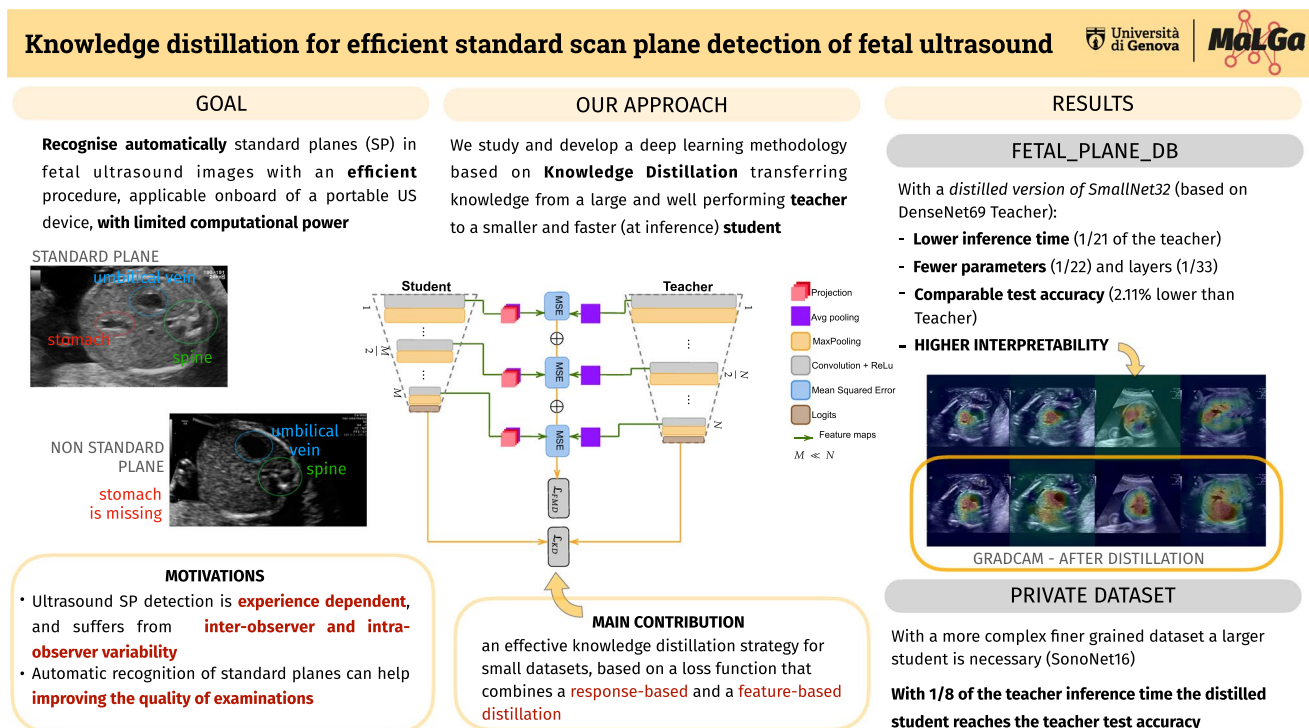

The original article has been corrected.

The original article can be found online at <https://doi.org/10.1007/s11517-023-02881-4>.

✉ Francesca Odone
 francesca.odone@unige.it
 Jacopo Daputo
 jacopo.daputo@edu.unige.it
 Luca Zini
 luca.zini@esaote.com

¹ MaLGA-DIBRIS, Università degli Studi di Genova, Genova, Italy
² Esaote S.p.A, Genova, Italy

Open Access This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not

permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>.

Publisher's Note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.